


Asthma Maintenance – Spirometry Workflow for Providers and Clinical Staff

Cerner PowerChart Ambulatory EDUCATION


Summary: Asthma Maintenance Screening is recommended every two years, for all patients with an Asthma diagnosis. This health maintenance recommendation will automatically display on the Recommendations component within the Ambulatory Workflow page every two years.

Support: Ambulatory Information at 231-392-0229

Managing Asthma Recommendation Workflow

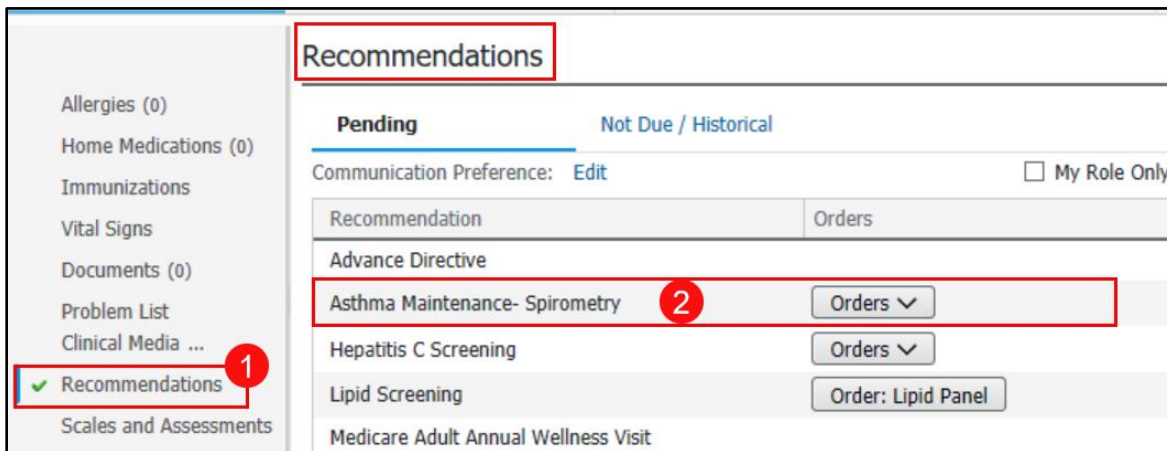

1. When a patient presents for an office visit, navigate to the Recommendations component of the Ambulatory Workflow page.
 - a. Check if the patient is due for an asthma maintenance screening.
2. If the patient is due for a screening, ask the patient if they have been screened for asthma in the last two years.
3. If the patient has not been screened for asthma in the last two years, proceed with the recommended Asthma Maintenance - Spirometry.

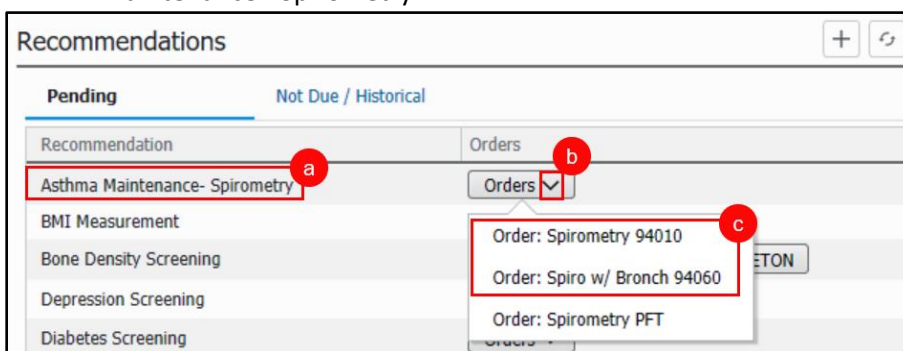

- a. Locate the Asthma Maintenance – Spirometry recommendation.
- b. Click the arrow beside Orders.
- c. Select the desired Order.

Note:

- Spirometry PFT – Testing occurs outside the ambulatory office (used the most common, as many offices have not restarted spirometry following COVID).
- Spirometry 94010; Spiro w/ Bronch 94060 – Testing that occurs inside the ambulatory office.

Asthma Maintenance – Spirometry Workflow for Providers and Clinical Staff

Cerner PowerChart Ambulatory EDUCATION

d. Click the Orders for Signature icon.



e. Complete Ordering Physician details by selecting:

1. Order.
2. Correct Physician.
3. Cosign Required.
4. Okay.

f. Select Modify Details.

Asthma Maintenance – Spirometry Workflow for Providers and Clinical Staff

Cerner PowerChart Ambulatory EDUCATION

The screenshot shows the 'Orders for Signature' section in Cerner PowerChart. The top navigation bar includes 'Add', 'Document Medication by Hx', 'External Rx History', and 'Rx Plans (0): In Process'. The 'Reconciliation Status' section shows 'Meds History', 'Admission', and 'Outpatient'. The left navigation pane is expanded to 'Orders for Signature'. The main area displays a table of orders for signature, with the 'Spirometry 94010' order selected. Below the table, the 'Details for Spirometry 94010' section is visible, showing 'Available Diagnoses' with 'Asthma (J45.909)' selected. A red box highlights the 'Sign' button, and a red circle 'g' highlights the 'Asthma (J45.909)' diagnosis.

- g. Select the patient’s current asthma diagnosis.
- h. Click Sign.

Outside Records Document of Asthma Maintenance - Spirometry

1. Navigate to the Recommendations component of the Ambulatory Workflow page.


The screenshot shows the 'Recommendations' window in Cerner PowerChart. The 'Pending' tab is active, and the 'Asthma Maintenance- Spirometry' recommendation is selected. A red box 'a' highlights the recommendation name. A red box 'b' highlights the 'Actions' dropdown menu, and a red box 'c' highlights the 'Completed' option in the dropdown.

- a. Click on Asthma Maintenance – Spirometry, from the recommendations list and the side window will open.
- b. Click the Actions drop down.
- c. Select Completed.

Asthma Maintenance – Spirometry Workflow for Providers and Clinical Staff

Cerner PowerChart Ambulatory EDUCATION

- d. Enter the date of the procedure was performed.
- e. Remove your name from the Recorded for field by clicking X. Add the provider's name if known. Leave blank if unknown.
- f. Enter a comment as needed.
- g. Click Save.

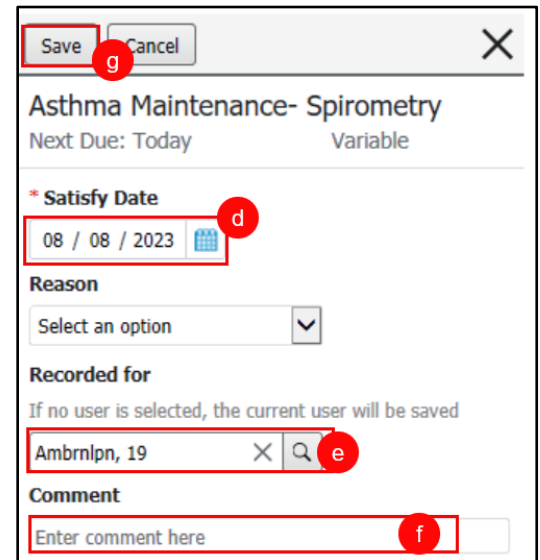

The screenshot shows a form titled "Asthma Maintenance- Spirometry" with the following fields and annotations:

- Save** button: Annotate with **g**.
- Satisfy Date**: A date field containing "08 / 08 / 2023" with a calendar icon. Annotate with **d**.
- Reason**: A dropdown menu with "Select an option" and a downward arrow.
- Recorded for**: A field containing "Ambrlnp, 19" with an "X" button and a search icon. Annotate with **e**.
- Comment**: A text input field with the placeholder "Enter comment here". Annotate with **f**.